
WalkingVest

SystemRoMedic

Trial Fitting Protocol



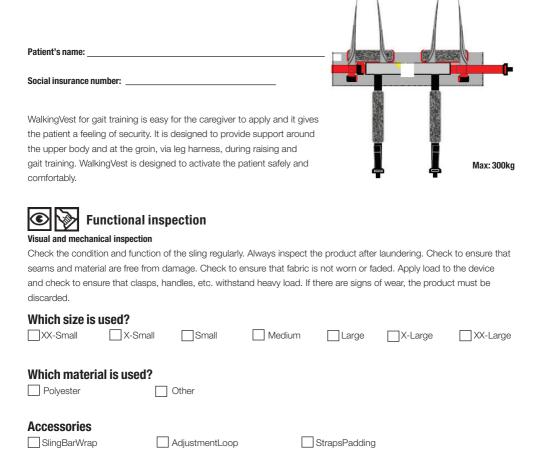

What is the width of the slingbar?

Instructions for use		
Can the sling/vest be used for transfers to/from the toilet?	Yes	No
Can the sling/vest be used in showering situations?	Yes	No
In which situations will the WalkingVest be used?	Yes	No
AdjustmentLoop:		
Have staff that use the assistive device: Read the instructions?	No No	
Instructions to personnel:		
e.g.; Placement of head/arms/hands? Placement of legs/feet? Use bed functions	S.	
Number of caregivers:		
Instructions to patient:		
e.g.; In what way can the patient participate actively in the transfer situation? Which	ch instruction	ons are used?
Other:		
Trial-fitted by:	Date:	

Handicare AB Veddestav. 15, Box 640 SE-175 27 Järfälla SWEDEN

Tel: +46 (0)8-557 62 200 Fax:+46 (0)8-557 62 299 E-mail: info@handicare.se

Internet: www.handicare.com

In the events of changes or questions, contact the trial-fitter.

Phone: Phone:

Manuals and instructions for functional testing are available on Handicare's website www.handicare.com

